


Shenzhen Well.D Medical Electronics Co., Ltd.

Address: Well.D Park Qinglan 3 Rd., National Biopharmaceutical Industrial Base

Pingshan New Area, Shenzhen , China, 5181
Telephone: +86-755-36900018/26073350

5 3 10 11

Website: www.welld.com.cn www.welld.net

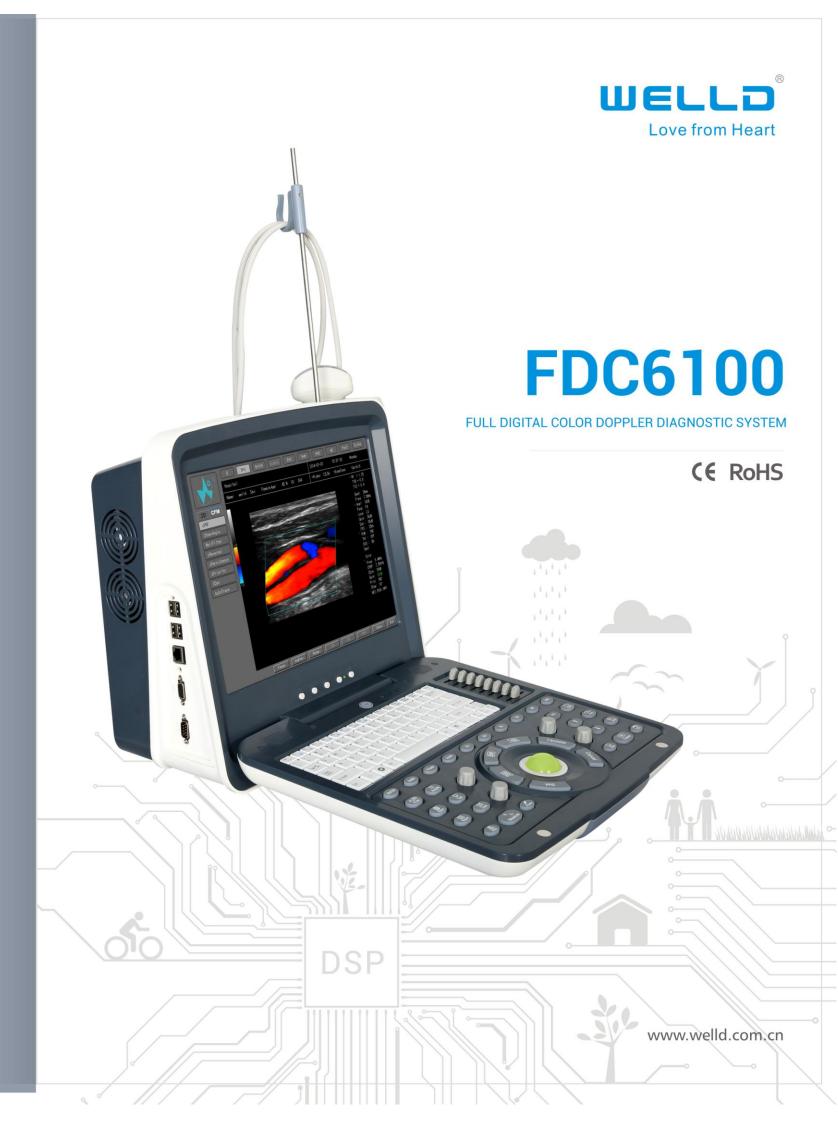

FDC6100 is a newly developed Color Doppler Diagnostic System of WELLD with completely independent intellectual property rights. Characterizing world-advanced technology, modern ergonomic design, stellar image quality, high blood sensitivity and extensive probe adaptation capability, it can meet varies needs of clinical diagnosis of abdomen, obstetrics, gynecology, cardiology, small organs, superficial blood vessels, musculoskeletal, ophthalmology, anesthesiology, urology, neurosurgery and other specialist clinics.

Leading Ultrasound Imaging Technology

1. World-advanced ultrasound platform and architecture

An 8-core DSP processor and a front-end ultrasound chip with the latest generation of "digital demodulator" is adopted, providing powerful computing capability, high integration, low power consumption as well as seamless upgrade which supports elastography.

2. Sparse transmit & multi-beam parallel processing technology

Plane-wave transmitting as well as 16-beam parallel receiving and processing improve the frame rate of image and blood sensitivity in B + C and B + C + D modes, achieving triplex display.

3. Pulse inversion harmonic imaging technology

Superior to traditional tissue harmonic imaging technology, pulse inversion harmonic imaging technology is applied to suppress side lobes and improve contrast resolution of the tissue with counteracted fundamental and enhanced harmonic.

4. Synthetic aperture beam-forming technology

Break of restrictions traditional DAS beam-forming algorithm has on the number of physical channels generates excellent images both in near field and in far field with smaller hardware and lower transmit power.

5. A continuous transmit focus at every pixel

The distance differences of transmitting sound waves and those of receiving sound waves are calculated simultaneously, resulting to higher imaging precision and accuracy. Diagnostic differences caused by differentiation of operators are lessened with no focus displayed and no need of manual adjustments.

6. Speckle noise suppression technology

Removal of speckle noise significantly clears and smooths the 2D image.

7. Freehand 3D & 4D imaging technology

The detection rate of fetal malformation is raised substantially.





Ergonomic Design



Operation panel characterizing numerical control back light, fast regulation and one-key easy optimization



Newly designed ergonomic appearance with a 15 inch LCD screen



Three probe connectors, free probe switching, hot-swapping available




DICOM3.0, remote network assistance available



Multiple choices of language display




Graphic workstations, import from and export to typical cases generating quick diagnosis



Optional lithium battery



Hidden handle

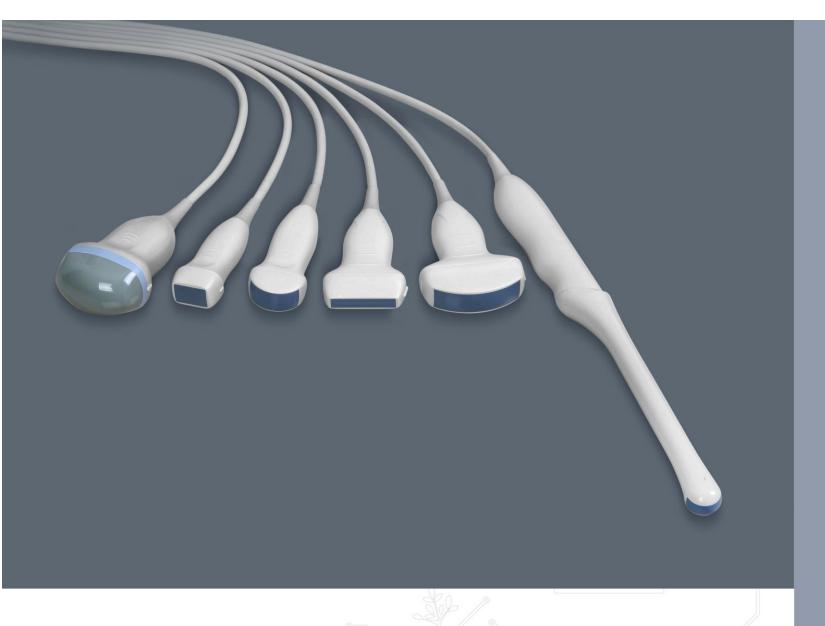

Broadband Frequency Probes

- High-density and wide-band probe group
- All probes supporting harmonic imaging mode









Vagina In Color Doppler Mode




2D Image - Twins




Thyroid In Color Doppler Mode




Vein Expansion And Reflux




Real-time Triplex Display




Reflux In Spectral Doppler




Communis Carotid Artery Biurcate In Color Doppler Mode




Cardiology In Color Doppler Mod



Abdomen In Color Doppler Mode



Real- time Triplex Display



Cardiology In Color Doppler Mode